



Instructions for the MonitorMark™ Time Temperature Indicators (#8201-01, 8205-01, 8207-01 & 8208-01)

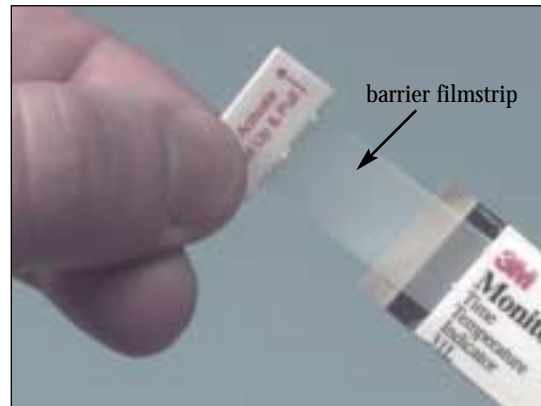

To activate indicators for use:
1. Fold up on the perforated activation tab located on the left side of the indicator.

2. Pull the activation tab out and the attached barrier filmstrip will come with it. The indicator is now ready to monitor temperatures.

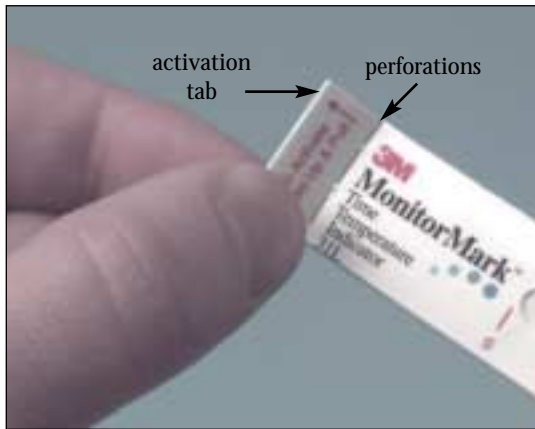

Attachment instructions: Peel the tan backing from the indicator until the white adhesive area is exposed. Press the white adhesive onto a clean, dry area by applying pressure to the indicator.

